



Bag Feed Set



Instructions for Use

The Vesco Q Enteral Feeding Pump® System is intended to be used by healthcare professionals, patients and caregivers for the intermittent and continuous delivery of enteral fluids for adult and pediatric (infant, child, and adolescent) feeding therapy in hospital and homecare environments.


Precautions:

- Failure to follow correct preparation of the pump set can negatively affect the accuracy of the enteral infusion system.
- Feed sets cannot be used for feeding programs for longer than 24 hours due to risk of bacterial contamination and system inaccuracy.


Directions:

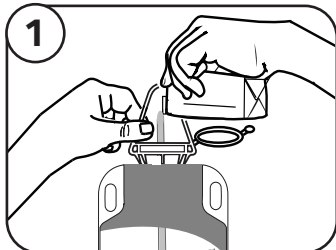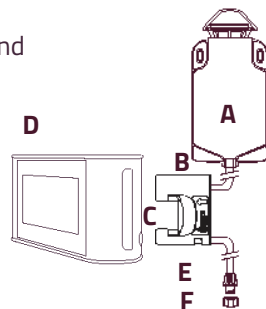


Fill bag (A) with desired or pre-scribed amount of enteral fluids.

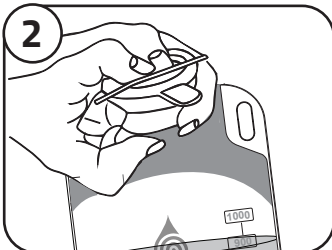


Securely close lid.

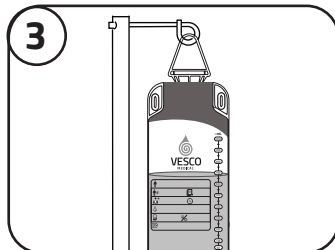


Hang bag on IV Pole 6 inches above top of pump.

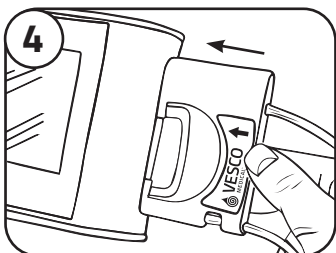

Insert cassette (B) into green opening (C) and click into place.

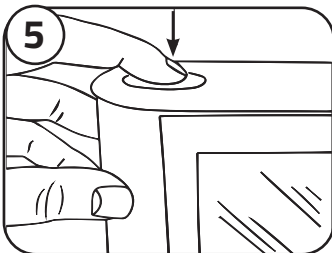

Press POWER button (D) on top of pump to power on.

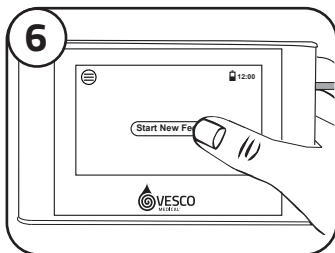


Touch START NEW FEED to initiate programming.

Scan
HERE




Scan for Additional Instructions on set-up and programming the pump.
or visit www.vescomedical.com/Q-resource-center


Directions (cont.):

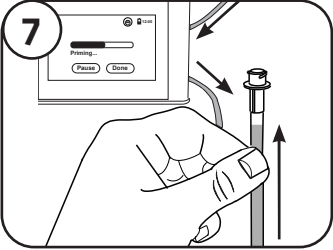

Remove dust cover (F) then prime to send nutrition to end of feed set.

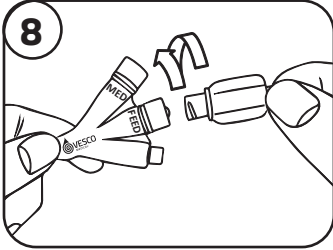

Attach distal female ENFit connector (E) to patient's male ENFit connector on feeding tube.

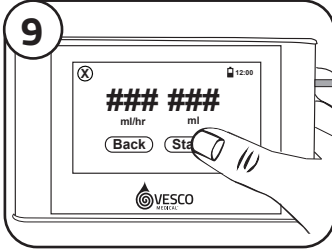

Run feed as programmed.

Note: This feed set is intended for use with the Vesco Q Enteral Infusion Pump to be used for enteral feeding therapy only. Approximate volume in milliliters.

Warnings:

- Feed set should not be misconnected with small bore connectors of other healthcare applications.
- Feed sets cannot be used for feeding programs longer than 24 hours because they cannot be adequately cleaned or sterilized for reuse, with risks of bacterial contamination, system inaccuracy, as well as bio-incompatibility from attempts.
- Use of feed sets longer than 24 hours risks bacterial contamination and negative effects on system accuracy.
- Do not use if package is opened or damaged.

Glossary of Symbols:

Do not reuse intended for single use	Do not use if package is damaged	Expiry date	Read Instructions for Use	Caution, consult accompanying documents	Non Sterile
Reference number	Lot Number	Date of manufacture	Prescription use only	(MR) Unsafe	Not for IV use
Keep away from sunlight	Keep dry	Manufacturer	Not made with BPA	Not made with phthalate plastcizers	Not made with natural rubber latex