

NEW

TwoPress® 2 Lite

Application Guide


ABI: 0.6 – 0.8

Visual
Indicators




2 Layer two:
Compression bandage


1 Layer one:
Padding bandage

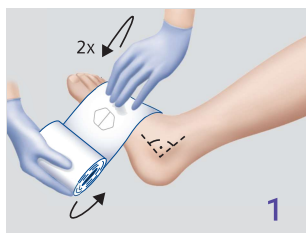


Ignoring the printed indicator, apply the white padding bandage (with the ink facing away from the skin), next to the base of the toes.

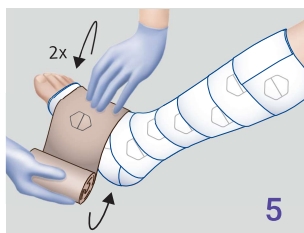


Ignoring the printed indicator, apply the cohesive compression bandage next to the base of the toes, so the edge of the white short-stretch padding remains visible.

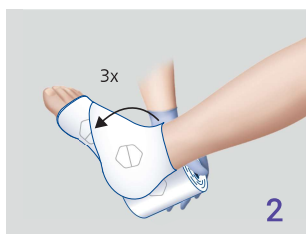


After two turns of fixation, wrap the bandage across the back of the foot and enclose the heel in figures of 8. Adjust the stretch based on the anatomy of the foot.

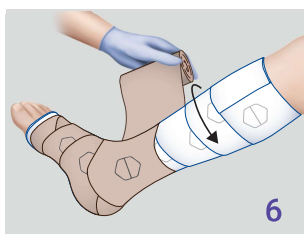


After two turns for fixation, wrap the bandage across the back of the foot and enclose the heel in figures of 8. Adjust the stretch based on the anatomy of the foot.

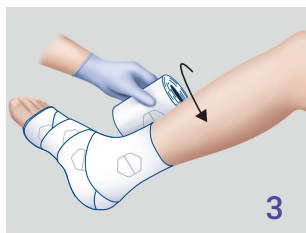


Using a spiral technique, wrap with an overlap of 50%. Stretch the bandage until the indicator shows a regular hexagon. Use the center line of the hexagon to guide overlap.

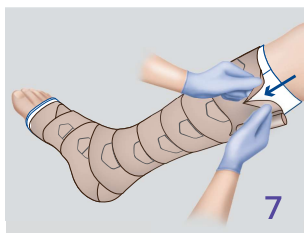

Using a spiral technique wrap with an overlap of 50%. Stretch the bandage until the indicator shows a regular hexagon. Use the center line of the hexagon to guide overlap. Tear off (pinch and pull) excess bandage material beneath the tibial tuberosity, leaving the edge of the white padding visible.

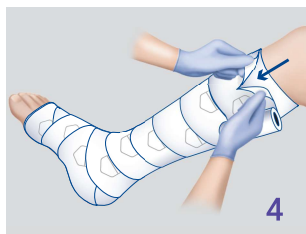

Tear off (pinch and pull) excess bandage material beneath the tibial tuberosity. Additional fixation is not necessary; tape may be used if desired.

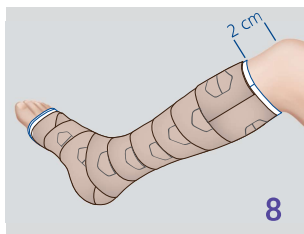

Press the compression bandage evenly with both hands over the entire lower leg.

For a detailed description of the application, please refer to the Instructions for Use.

Indicator Usage Guide



Contact your local HARTMANN representative, or visit us
at www.hartmannusa.com for more information.

HARTMANN USA, Inc.
Rock Hill, SC 29730
1-800-243-2294

www.hartmannusa.com

XLIT 2974 Rev. 2 (0921)

