



REF HCS70004P, HCS70004G
HCS70004C, HCS70004BL
HCS70004DP, HCS70004

AEROMIST COLORS™

NEBULIZER
COMPRESSOR KIT

Instruction Manual

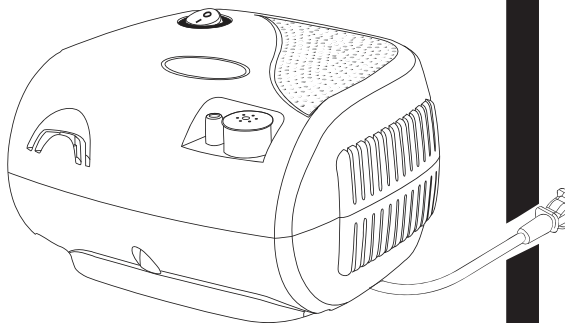







TABLE OF CONTENTS

IEC Symbols.....	2
Important Safeguards.....	2
Introduction.....	3
Specifications.....	4
Description.....	5
Operation Instructions.....	6
Cleaning.....	7
Maintenance.....	7
Trouble Shooting Guide.....	8
Warranty.....	9

IEC SYMBOLS

Caution, Attention or Consult accompanying documents.....	
Type BF Equipment.....	
Alternating Current.....	
Double Insulation.....	
Indoor Use Only.....	

IMPORTANT WARNINGS

Caution:

1. Federal Law (USA) restricts this device for sale or use on the order of a physician.
2. Follow the instructions of your physician to operate this unit.
3. This product is a nebulizer for the inhalation of medical aerosols and is suitable for all commonly used solutions. Use only the type and amount of medication prescribed by your doctor.
4. This product is intended for aerosol therapy only. Any other use is not recommended.
5. Do not untwist the jet nebulizer during operation.
6. Do not pour more than 10 mL of solution into the jet nebulizer.

Danger: To Reduce the risk of electrocution

7. Always unplug the unit immediately after using.
8. Do not use while bathing.
9. Do not place or store the unit where it can fall or be pulled into a tub or sink.
10. Do not place or drop into water or other liquid.
11. Do not reach for a product that has fallen into water. Unplug immediately.

 **Warning: To Reduce the risk of burns, electrocution, fire or injury**

1. Electrical Shock Hazard - do not remove the cabinet or open the cover.
2. Disconnect the power cord from the electrical outlet before cleaning or servicing.
3. Do not place this equipment near hot, sparking or burning objects
4. Do not use oil or grease on or near this device.
5. Turn the unit off when it is not in use.
6. Keep the cord away from HEATED or HOT surfaces.
7. NEVER drop or insert any object into any opening.
8. NEVER block the air openings of the product or place it on a soft surface, such as a bed or couch, where the air opening may be blocked.
9. Avoid operating in wet or damp locations.
10. Unplug the unit before filling the nebulizer.

 **Warning: To reduce the risk of infection:**

Cleaning of the nebulizer is recommended after each aerosol treatment. Disinfecting is recommended once a day. Please follow cleaning and disinfecting instructions in this manual.

INTRODUCTION


This compressor nebulizer is designed to deliver the prescribed medication solution to treat your respiratory disorders: such as asthma, allergies, and bronchitis. The nebulizer converts the medication solution into an aerosolized mist which is inhaled by the patient through the mouthpiece. Read this manual thoroughly before using the nebulizer and save for future reference.

SPECIFICATIONS

Items	HCS70004P, HCS70004G, HCS70004BL, HCS70004C, HCS70004DP, HCS70004
Current	120V/60HZ
Power consumption	180 VA Max
Nebulize Cup	#30503
Operation air pressure	9 - 16 Psi (62 - 110 kPa)
Max air pressure	35 - 50 Psi (241 - 345 kPa)
Operation Air Flow	5.0 - 8.0 Lpm
Nebulizer rate	≥ 0.18mL/min (2% saline)
Noise level	≤ 55 dB
Operation R.H.	30 - 85% RH
Operation temperature	10 - 40 °C (50 - 104 °F)
Storage R.H.	30 - 85% RH
Storage temperature	-20 - 70 °C (-4 - 158 °F)
Dimensions(L x W x H)	150 x 140 x 90 mm
Weight	1.2 kg

- (1). Conditions may vary based on altitude above sea level, barometric pressure air temperature. Specifications subject to change without notice.
- (2). Nebulizer specifications may vary with the kind of medication being used and its viscosity.
- (3). For electromagnetic compatibility the standards are based as follow: IEC/EN 60601-1-2.
- (4). Protection against electric shock is classified as Type II.
- (5). Degree of protection against electric shock is classified as Type BF.
- (6). Equipment not suitable for use in the presence of a flammable anesthetic mixture with air, oxygen, or nitrous oxide.

DESCRIPTION

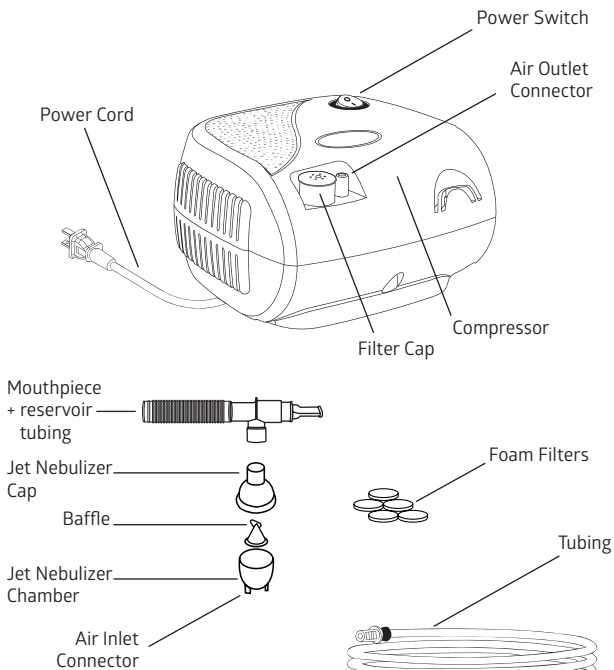

OPERATION INSTRUCTIONS

1. Place compressor on a stable, sturdy and flat surface such that the unit can be easily reached when you're seated.
2. Make sure the compressor is off by pressing the power switch to the "OFF" (O) position.
3. Plug power cord into a wall outlet.
4. Connect one end of the tubing into the compressor air outlet connector.
5. Add the prescribed solution through the opening on jet nebulizer cap using an eye dropper or pre-measured dose container.
6. Assemble mouthpiece onto the top of the jet nebulizer cap. If an aerosol mask is used, connect the bottom of mask to the top of jet nebulizer cap.
7. Connect tubing to jet nebulizer air inlet connector.
8. Turn the compressor on by pressing power switch to "ON" (I) position.
9. Implement the treatment by placing the mouthpiece between the teeth. Inhale and exhale through the mouthpiece.
10. If an aerosol mask is used, place the mask over the mouth and nose.

Note: The compressor motor has a thermal protector which will shut off the unit before the unit overheats. When the thermal protector shuts the unit off:

- 1) Switch off the unit, 2) Unplug the unit from the electrical outlet, 3) Wait 30 minutes for the motor to cool down before another treatment.

CLEANING

1. Turn the power off and unplug the compressor power cord from the wall outlet.
2. Remove the tubing from the air inlet.
3. TO CLEAN: Disassemble mouthpiece, jet nebulizer cap, chamber and baffle, and wash these items in hot water with dish-washing detergent. Rinse these items thoroughly to remove the detergent and let air dry.
4. TO DISINFECT: Mix 1/4 cup of white vinegar with 3/4 cup hot water in a clean container. Submerge mouthpiece, T-piece, nebulizer cap, chamber and baffle for 30 minutes in the solution. Remove from solution and let air dry.
5. There is no need to clean the tubing. If necessary wipe the surface regularly.

CAUTION: The jet nebulizer must be changed if it gets clogged.

CAUTION: The nebulizer and accessories must not be boiled.

MAINTENANCE

1. The air compressor filter should be replaced when it turns gray. Additional filters can be purchased from your dealer.
2. Only authorized personnel shall make repairs to this product.

CAUTION: The nebulizer may be damaged if used with a dirty filter or if the filter is replaced by other material such as cotton. Do NOT operate without a filter.

TROUBLE SHOOTING GUIDE

If a problem occurs during operation, please check and correct the following points:

SYMPTOM	POSSIBLE CAUSE	SUGGESTED SOLUTIONS
When switching it on, it does not work.	Incorrectly plugged.	Check if the unit is properly connected.
The mist does not come out from the jet nebulizer/ aerosol output reduced (low).	<ol style="list-style-type: none">1. Incorrect amount of medication in the jet nebulizer.2. Tubing disconnected.3. The jet nebulizer is not creating mist.4. The air filter is clogged.	<ol style="list-style-type: none">1. The jet nebulizer's maximum capacity is 10mL. Adjust the volume until the nebulizer functions correctly.2. Connect the tubing.3. Replace the jet nebulizer.4. Replace the air filter.

WARRANTY

Medline Industries, Inc. warrants the nebulizer compressor to be free from defective workmanship and materials for a period of (5) years from the date of purchase. Check with your dealer for more details. This warranty is limited to the original purchaser of the compressor. Any defective part or assembly will be repaired or replaced, at the sole discretion and determination of Medline Industries, Inc., if the unit has been properly operated during the warranty period. Normal maintenance items and disposable components are not covered by this warranty. Shipping charges, if any, shall be paid by the purchaser.

Note: There is no other express warranty. Implied warranties, including those of merchantability and fitness for a particular purpose, are limited to the duration of the express limited warranty and to the extent permitted by law and all implied warranties are excluded. This warranty does not cover providing a loaner compressor, compensating for costs incurred for compressor rental, or labor costs incurred in repairing or replacing defective part(s).

www.medline.com

Aeromist Colors™ is a trademark and Medline is a registered trademark of Medline Industries, Inc.
Manufactured for: Medline Industries, Inc.
Three Lakes Drive, Northfield, IL 60093 USA
Product of China. **1-800-MEDLINE** RD17ZBI